

# **TNF-alpha [Biotinylated]: TNFR2 Inhibitor Screening ELISA Kit**

**Pack Size: 96 tests**

**Catalog Number: EP-147**

**IMPORTANT: Please carefully read this manual before performing your experiment.**

***For Research Use Only. Not For Use In Diagnostic Or Therapeutic Procedures***

## **INTENDED USE**

This kit is designed for screening of inhibitors of binding between human TNF-alpha and human TNFR2.

It is intended for research use only (RUO).

## **PRINCIPLE OF THE ASSAY**

This inhibitor screening ELISA kit is designed to facilitate the identification and characterization of new TNF-alpha pathway inhibitors. The assay takes advantage of our in house-developed binding of biotinylated human TNF-alpha to immobilized human TNFR2 in a functional ELISA assay, and employs a simple colorimetric ELISA platform.

Briefly, we provide you with a human TNFR2 protein, a Biotinylated human TNF-alpha, an anti- TNF-alpha neutralizing antibody (as method verified Std.), and Streptavidin-HRP reagent. Your experiment will include 4 simple steps:

- 1) Coat the plate with human TNFR2.
- 2) Add your molecule of interest to the tests.
- 3) Add human TNF-alpha-Biotin to bind the coated human TNFR2.
- 4) Add Streptavidin-HRP followed by TMB or other colorimetric HRP substrate.

Finally, the half maximal inhibitory concentration (IC50) of your compound to TNF-alpha: TNFR2 binding will be determined by comparing OD readings among different experimental groups.

## **MATERIALS PROVIDED**

**TABLE 1. MATERIALS PROVIDED (pls modify according to COA)**

| Catalog   | Components                            | Size<br>(96 tests) | Format | Storage            |  |
|-----------|---------------------------------------|--------------------|--------|--------------------|--|
| EP147-C01 | High-bind Plate                       | 1 plate            | Solid  | 2-8°C              |  |
| EP147-C02 | Human TNFR2                           | 15 µg              | Powder | 2-8°C              | -70°C after<br>reconstitution, avoid<br>freeze-thaw cycles |
| EP147-C03 | Biotinylated Human TNF-alpha          | 10 µg              | Powder | 2-8°C              |  |
| EP147-C04 | Anti- TNF-alpha Neutralizing Antibody | 20 µg              | Powder | 2-8°C              |  |
| EP147-C05 | Streptavidin-HRP                      | 10 µg              | Powder | 2-8°C, avoid light |  |
| EP147-C06 | Coating Buffer                        | 12 mL              | Liquid | 2-8°C              |  |
| EP147-C07 | 10xWashing Buffer                     | 50 mL              | Liquid | 2-8°C              |  |
| EP147-C08 | Blocking Buffer                       | 50 mL              | Liquid | 2-8°C              |  |
| EP147-C09 | Substrate Solution                    | 12 mL              | Liquid | 2-8°C, avoid light |  |
| EP147-C10 | Stop Solution                         | 7 mL               | Liquid | 2-8°C              |  |

### **REAGENTS/EQUIPMENT NEEDED BUT NOT SUPPLIED**

Single or dual wavelength microplate reader with 450 nm/630nm filter;

Centrifuge;

37 °C Incubator;

Single channel or multichannel pipettes with 10 µL, 200 µL and 1000 µL precision;

10 µL, 200 µL and 1000 µL pipette tips;

Test Tubes;

Graduated cylinder;

Deionized or distilled water for dilution;

### **STORAGE AND VALIDITY INSTRUCTIONS**

Unopened kit should be stored at 2°C -8°C upon receiving. Find the expiration date on the outside packaging and do

not use reagents past their expiration date.

The kit should be stored as TABLE 1 after the reconstitution of lyophilized materials. The shelf life is 30 days from the date of opening.

*Note:*

- a. Do not use reagents past their expiration date.
- b. Find the expiration date on the outside packaging.

**REAGENT PREPARATION**

1. Restore all reagents and samples to room temperature (20-25°C) before use.
2. Reconstitute the provided lyophilized materials to stock solutions with sterile deionized water as recommended in Tab.2, Solubilize for 15 to 30 minutes at room temperature with occasional gentle mixing. Avoid vigorous shaking or vortex. The reconstituted stock solutions should be stored at -70°C. **Avoid freeze-thaw cycles.**

*Note: Streptavidin-HRP stock solution should be protected from light.*

TABLE 2. RECONSTITUTION METHODS FOR 96 TESTS

| Catalog   | Components                            | Amount | Stock Solution Con. | Reconstitution Buffer and Vol. |
|-----------|---------------------------------------|--------|---------------------|--------------------------------|
| EP147-C02 | Human TNFR2                           | 15 µg  | 100 µg/mL           | 150 µL, water                  |
| EP147-C03 | Biotinylated Human TNF-alpha          | 10 µg  | 50 µg/mL            | 200 µL, water                  |
| EP147-C04 | Anti- TNF-alpha Neutralizing Antibody | 20 µg  | 100 µg/mL           | 200 µL, water                  |
| EP147-C05 | Streptavidin-HRP                      | 10 µg  | 50 µg/mL            | 200 µL, water                  |

**RECOMMENDED PROTOCOL**

**1. Working solution preparation**

1.1 Preparation of 1×Washing Buffer:

Dilute 50 mL 10×Washing Buffer with ultrapure water/deionized water to 500 mL.

1.2 Preparation of Dilution Buffer:

10 mL Blocking Buffer (EP147-C08) add 30 mL 1×Washing Buffer.

**2. Coating**

1) Dilute Human TNFR2 stock solution (100 µg/mL) to 1 µg/mL with Coating Buffer to make Human TNFR2 working solution.

2) Add 100 µL of Human TNFR2 working solution (1 µg/mL) to each well and leave a couple of wells uncoated for No-Coating Control, seal the plate with microplate sealing film and incubate overnight (or 16 hours) at 4°C.

### 3. Washing

Remove the remaining solution by aspiration, add 300 µL of 1×Washing Buffer to each well, gently tap the plate for 1 minute, remove any remaining 1×Washing Buffer by aspirating or decanting, invert the plate and blot it against paper towels. Repeat the washing step above for three times.

*Note: For best results, the complete removal of the Human TNFR2 solution is essential. The use of a manifold dispenser or an auto-washer may be necessary.*

### 4. Blocking

Add 300 µL Blocking Buffer to each well, seal the plate with microplate sealing film and incubate at 37°C for 1.5 hours.

### 5. Washing

Repeat step 3. At the same time, you can start to prepare your samples.

### 6. Add Samples

1) Make serial dilution of the samples as appropriate.

2) If you intend to use the provided Anti-TNF-alpha Neutralizing Antibody as a reference (Std.), you may dilute the antibody as recommended in Figure 1.

3) Add 50 µL of sample solution to each well according to our recommendation (Figure 2) or your own plate setup.

4) For No-Coating Control wells, please add 50 µL Dilution Buffer.

### 7. Binding

1) Dilute Biotinylated Human TNF-alpha stock solution (50 µg/mL) to 0.05 µg/mL with Dilution Buffer to make Biotinylated Human TNF-alpha working solution.

2) For No-binding control wells, please add 50 µL Dilution Buffer.

3) For all other wells, please add 50 µL Biotinylated Human TNF-alpha working solution to the wells and mix the


samples by gently tapping the plate. Seal the plate with microplate sealing film and incubate at 37°C for 1 hour.

**Note: The working solution should be prepared immediately before use and should not be stored.**

**FIG.1 PREPARATION OF 1:1 SERIAL DILUTIONS OF THE Anti-TNF-alpha Neutralizing Antibody**

| Tubes/<br>Solution<br>Code | Anti-TNF-alpha<br>Neutralizing<br>Antibody<br>stock solution | Std.-1      | Std.-2     | Std.-3       | Std.-4        | Std.-5         | Std.-6         | Std.-7         | Std.-8         | Std.-9         | Std.-10         |
|----------------------------|--|-------------|------------|--------------|---------------|----------------|----------------|----------------|----------------|----------------|-----------------|
| Operating                  |  | 200 µL      | 200 µL     | 200 µL       | 200 µL        | 200 µL         | 200 µL         | 200 µL         | 200 µL         | 200 µL         | 200 µL          |
| Solution<br>Con.           | 100 µg/mL  | 10<br>µg/mL | 5<br>µg/mL | 2.5<br>µg/mL | 1.25<br>µg/mL | 0.625<br>µg/mL | 0.312<br>µg/mL | 0.156<br>µg/mL | 0.078<br>µg/mL | 0.039<br>µg/mL | 0.0195<br>µg/mL |
| Dilution<br>Buffer Vol.    |  | 360 µL      | 200 µL     | 200 µL       | 200 µL        | 200 µL         | 200 µL         | 200 µL         | 200 µL         | 200 µL         | 200 µL          |

**FIG.2 PLATE LAYOUT**

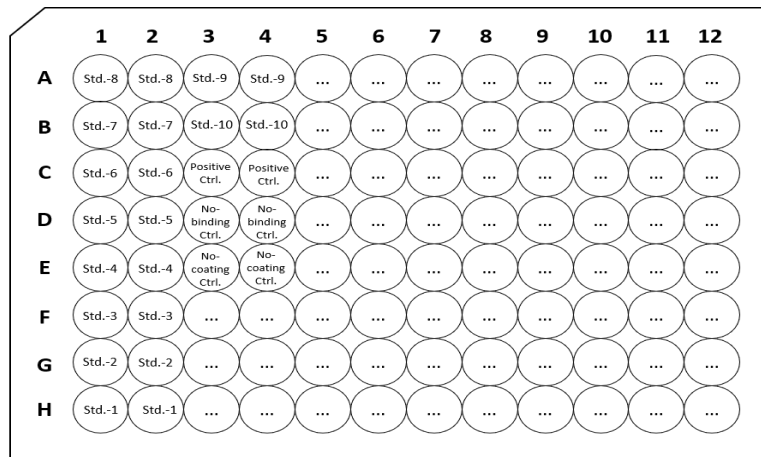

### 8. Washing

Repeat step 3.

### 9. Add Streptavidin-HRP

1) Dilute Streptavidin-HRP stock solution (50 µg/mL) to 0.1 µg/mL with Dilution Buffer to make Streptavidin-HRP working solution.

2) For all wells, add 100 µL Streptavidin-HRP working solution, seal the plate with microplate sealing film and incubate at 37°C for 1 hour, avoid light.

## 10. Washing

Repeat step 3.

## 11. Substrate Reaction

Add 100  $\mu$ L **Substrate Solution** to each well. Seal the plate with microplate sealing film and incubate at 37°C for 20 minutes. Avoid light.

## 12. Termination

Add 50  $\mu$ L **Stop Solution** to each well, and gently shake the plate to allow thorough mixing.

*Note: the color in the wells should change from blue to yellow.*

## 13. Data Recording

Read the absorbance at 450 nm using UV/Vis microplate spectrophotometer.

*Note: Subtracting the value read at OD<sub>450nm</sub> with OD<sub>630nm</sub> can be used to reduce the background noise.*

## SIMPLIFIED PROTOCOL

TABLE. 3 ASSAY PROTOCOL

| Steps Code | Steps                     | Reagents & Instruments                        | Reaction Conditions                                 | Samples     | No-binding Ctrl. | No-coating Ctrl. | Positive Ctrl. |
|------------|---------------------------|---|---|-------------|------------------|------------------|----------------|
| 1          | Working fluid preparation | N/A   | N/A   | N/A         | N/A              | N/A              | N/A            |
| 2          | Coating                   | Human TNFR2 Working Solution                  | 4°C for overnight                                   | 100 $\mu$ L | 100 $\mu$ L      | —                | 100 $\mu$ L    |
| 3          | Washing                   | 1X Wash Buffer                                | Wash for 3 times                                    | 300 $\mu$ L | 300 $\mu$ L      | 300 $\mu$ L      | 300 $\mu$ L    |
| 4          | Blocking                  | Blocking Buffer                               | 37°C for 1.5 hours                                  | 300 $\mu$ L | 300 $\mu$ L      | 300 $\mu$ L      | 300 $\mu$ L    |
| 5          | Washing                   | 1X Wash Buffer                                | Wash for 3 times                                    | 300 $\mu$ L | 300 $\mu$ L      | 300 $\mu$ L      | 300 $\mu$ L    |
| 6          | Add Samples               | Samples                                       | —   | 50 $\mu$ L  | —                | —                | —              |
|            |                           | Dilution Buffer                               |   | —           | 50 $\mu$ L       | 50 $\mu$ L       | 50 $\mu$ L     |
| 7          | Binding                   | Biotinylated Human TNF-alpha Working Solution | Mix by gentle tapping, incubate at 37°C for 1 hours | 50 $\mu$ L  | —                | 50 $\mu$ L       | 50 $\mu$ L     |
|            |                           | Dilution Buffer                               |   | —           | 50 $\mu$ L       | —                | —              |

|    |                    |                                   |  |        |        |        |        |
|----|--------------------|-----------------------------------|--|--------|--------|--------|--------|
| 8  | Washing            | 1XWash Buffer                     | Wash for 3 times   | 300 µL | 300 µL | 300 µL | 300 µL |
| 9  | Streptavidin-HRP   | Streptavidin-HRP Working Solution | 37°C for 1 hours   | 100 µL | 100 µL | 100 µL | 100 µL |
| 10 | Washing            | 1XWash Buffer                     | Wash for 3 times   | 300 µL | 300 µL | 300 µL | 300 µL |
| 11 | Substrate Reaction | Substrate Solution                | 37°C for 20 minutes  | 100 µL | 100 µL | 100 µL | 100 µL |
| 12 | Termination        | Stop Solution                     | Mix by gentle tapping  | 50 µL  | 50 µL  | 50 µL  | 50 µL  |
| 13 | Data Recording     | UV/Vis spectrophotometer          | Measure absorbance at 450 nm, with the correction wavelength set at 630 nm |        |        |        |        |

**Note for TAB. 3:**

- 1) *Samples: Your samples of interest.*
- 2) *No-binding Ctrl.: Reaction without Biotinylated Human TNF-alpha added. The absorbance should be around 0.05(< 0.1) at 450 nm.*
- 3) *No-coating Ctrl.: Reaction without Human TNFR2 coated on the wells. The absorbance should be around 0.05(< 0.1) at 450 nm.*
- 4) *Positive Ctrl.: Determined the max value in 450nm absorbance, when out of inhibitors.*
- 5) *It is recommended that all samples, controls and standards should be done in duplicates.*

**PRECAUTIONS**


1. This kit is for research use only and is not for use in diagnostic or therapeutic applications.
2. This kit should be used according to the provided instructions.
3. Do not mix reagents from different lots.
4. All reagents should be balanced to room temperature (20°C-25°C) before use.
5. This kit should be stored at 2°C-8°C.
6. Please prepare the working solution of each component according to the needs of the experiment. Except for 1x Washing Buffer, all prepared working solution is for one-time use and cannot be stored.

**METHOD VERIFICATION**

**INHIBITION OF TNF-alpha [Biotinylated]: TNFR2 BINDING BY ANTI- TNF-alpha NEUTRALIZING ANTIBODY**



Serial dilutions of Anti- TNF-alpha Neutralizing antibody (Catalog # EP147-C04) (1:1 serial dilution, from 10 µg/mL to 0.02µg/mL) was added into Biotinylated TNF-alpha: TNFR2 binding reactions. The assay was performed according to the protocol described below. Background was subtracted from data points prior to log transformation and curve fitting.

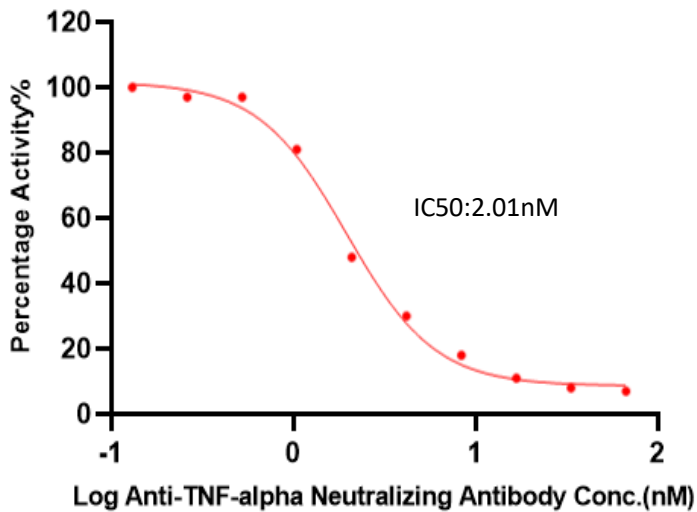

| Anti-TNF-alpha Neutralizing Antibody Conc.(µg/ml) | Anti-TNF-alpha Neutralizing Antibody Conc.(nM) | Mean Abs.(OD450) | Percentage Activity(%) |
|---|--|------------------|------------------------|
| 0   | 0.000  | 2.724            | 100%                   |
| 0.020   | 0.130  | 2.717            | 100%                   |
| 0.039   | 0.260  | 2.64             | 97%                    |
| 0.078   | 0.521  | 2.644            | 97%                    |
| 0.156   | 1.042  | 2.205            | 81%                    |
| 0.313   | 2.083  | 1.318            | 48%                    |
| 0.625   | 4.167  | 0.808            | 30%                    |
| 1.25  | 8.333  | 0.494            | 18%                    |
| 2.5   | 16.667   | 0.306            | 11%                    |
| 5   | 33.333   | 0.207            | 8%                     |
| 10  | 66.667   | 0.181            | 7%                     |
| No Coating  |  | 0.058            |                        |
| No Binding  |  | 0.053            |                        |

**For each experiment, a standard curve needs to be set for each micro-plate, and the specific OD value may vary depending on different laboratories, testers, or equipments. The example data is for reference only.**